



H₂HUBB TEST REPORT

Overland Park KS
 Info@H₂HUBB.com
 www.H₂HUBB.com

Date : 19 Jan 2026

Evaluation Introduction

Our report summarizes our analysis of the Nexis - Professional Hydrogen Water Bottle offered by the company Ocemida. H₂HUBB classifies this device as a premium high-pressure (psi) H₂ water portable system. The device features a PEM/SPE membrane to ensure H₂ gas production regardless of source water conductivity (TDS). Its session time-frame or cycle time-frames are 5 minutes and 10 minutes. We evaluated the system's dissolved hydrogen performance at 5 and 10 minutes. The unit contains a 3.7 V +1650 mAh battery, as stated by the battery specs. Our investigation was to analyze whether the product would meet our H₂ product performance standards, which must be achieved to be approved and recommended by H₂HUBB.

To learn more about our H₂ performance standards for hydrogen water bottles, visit [H₂HUBB](#).

H₂ Products

- Company: Ocemida
- Product Name: Nexis - Professional Hydrogen Water Bottle
- Type: High-Concentration H₂ Water Device
 - PEM/SPE
 - Portable Hydrogen Water Generator
 - High-PSI bottle
- URL Link: <https://ocemida.com>

Method and Procedure

- Distilled water: 6.0 pH (verifies that unit can function with low water conductivity)
- ΔpH (delta pH): Did not increase
- Water Temperature: 65~70°F/ 18~21°C
- Bottle Vol Size: 0.270 L or 270 mL (9.12 oz)
- Cycle Time Frame:
 - 5-minutes
 - 10-minutes
- Contamination Tests:
 - Chlorine generation (Cl₂)
 - Ozone Generation (O₃)
- Test Location: 277 meters (909 ft elevation)
- Test Methodology:
 - Electrochemical detection using Unisense H₂ Microsensor.
- All Dissolved H₂ Concentration Tests Converted to SATP (water temp and pressure)
- Claimed Dissolved H₂ mg/L: > 6.0 mg/L as stated on packaging



Test Results

To measure the dissolved hydrogen gas concentration, the **Nexis** Bottle was filled with 270 mL (9.12 oz) of distilled water—up to the base of the lid threads. The lid was then securely fastened, and the system was activated using either the 5-minute or 10-minute hydrogen generation mode. All measurements were conducted using the **Unisense H₂ Microsensor** paired with the **UniAmp** amplifier. Each test was performed in triplicate to ensure accuracy and reproducibility, and the resulting values were averaged to determine the bottle's overall performance. While the primary focus is on the mean dissolved hydrogen concentration, peak concentration values are also reported to provide a more comprehensive assessment of the bottle's hydrogen-generation capability.

H₂ Concentration at SATP:

- 5-mins avg mg/L (ppm): $\cong 5.40$ mg/L (ppm)
- 10-mins avg mg/L (ppm): $\cong 7.70$ mg/L (ppm)

Peak H₂ Concentration at SATP:

- 5-mins peak mg/L (ppm): $\cong 5.53$ mg/L (ppm)
- 10-mins peak mg/L (ppm): $\cong 7.83$ mg/L (ppm)

Avg H₂ mg Produced in Designated Vol:

- 5-mins: $\cong 1.46$ mg ($\equiv 17.72$ mL Dissolved)
- 10-mins: $\cong 2.08$ mg ($\equiv 25.25$ mL Dissolved)
- **Claimed H₂ mg/L (ppm) confirmed: Yes**

H₂HUBB Hydrogen Concentration Assessment

- According to our testing, the **Nexis** - Professional Hydrogen Water Bottle consistently achieved dissolved molecular hydrogen concentrations ranging from 5.40 to 7.70 mg/L (ppm) during both the 5- and 10-minute generation cycles, with a peak concentration of 7.83 mg/L (ppm) measured using the **Unisense H₂ Microsensor**. Based on current human clinical literature, these concentrations are sufficient to provide therapeutic benefits. The device exceeds H₂HUBB's performance standards for both **H₂ Concentration and Daily Dose of H₂**. For practical use, we recommend the 10-minute cycle as the optimal dose and setting for preparing hydrogen-rich water with this bottle.

Contamination Test:

- Chlorine (Cl₂): No detectable levels
- Ozone (O₃): No detectable levels

Internal Performance

Manufacturer's Rated Electrical Values: (as stated on the power supply)

- **Type of device/electrolytic cell**
 - Pure H₂; PEM/SPE membrane
- **Applied volts:**
 - 3.7 volts
- **Total Amps:**
 - 1650 mAh (1.65 amps)
- **Total watts:**
 - 6.10 Wh (watts)



Product Assessment

Functionality:

- Power on/off button
 - Located on the H₂ generator.
 - Press the power button to initiate electrolysis for hydrogen gas production and initiate a 5-minute session, then shuts off.
 - Press the power button twice to initiate a 10-minute session time then shuts off.
- USB-C charging port
 - Located on the backside of the device.
- Anode reservoir off-gas port
 - Pin-hole located on the bottom of the bottle.

Reliability:

- New: Yes
 - Initial test results and evaluation are currently on the report. (see Overall Opinion)

Overall Opinion

The NEXIS – Professional Hydrogen Water Bottle from Ocemida is a well-constructed, high-pressure (high-PSI) hydrogen water generator designed to produce exceptionally high concentrations of dissolved molecular hydrogen. In H₂HUBB's evaluation, a 10-minute operation cycle produced an average dissolved hydrogen concentration of 7.70 mg/L (ppm) in 270 mL (9.12 oz) of water, corresponding to a total hydrogen content of 2.08 mg, or approximately 25.25 mL of H₂ gas at SATP. The device also achieved a peak hydrogen concentration of 7.83 mg/L, demonstrating its ability to exceed the 6.0 mg/L threshold—an emerging benchmark among the highest-performing hydrogen water bottles currently available.

It is important to note that H₂HUBB documents maximum peak concentrations for reference purposes only and does not interpret these values as concentrations that can be consistently achieved. For this reason, our reports prioritize average dissolved hydrogen concentrations derived from multiple replicate measurements, as these values provide a more reliable indicator of sustained performance and consistency. Dissolved hydrogen levels were measured using a Unisense H₂ Microsensor with UniAmp amplifier, a laboratory-grade electrochemical system offering real-time detection and precision comparable to gas chromatography, while minimizing the variability commonly observed with colorimetric (oxidimetry-based) testing methods.

Dissolved hydrogen concentration (mg/L (ppm)) is a critical performance metric, as research suggests that 1-3 mg of H₂ or more per day appears to be therapeutic for humans. Furthermore, the IHSA standard for this type of product is a minimum of 0.5 mg/serving or 0.5 mg/L. H₂HUBB's performance standard for hydrogen water devices is slightly higher than IHSA, as we require the device to provide a concentration of 0.8 mg/L (ppm) and 0.8 mg/day consistently. The NEXIS Hydrogen Water Bottle offered by Ocemida surpassed H₂HUBB standards for both H₂ Concentration and Daily Dose of H₂. Based on current research data, we believe the device's mg/L (ppm) performance provides adequate levels of hydrogen gas to induce therapeutic effects in humans. **According to our test results, the product will be able to easily provide 1-3 mg of H₂ per day.** We are pleased with the device's dissolved hydrogen concentration.

Additionally, H₂HUBB employed a specialized PEM membrane conditioning ("break-in") protocol for this bottle prior to formal testing. Our standard conditioning procedure involves multiple warm-water soak cycles combined with repeated device activation to hydrate and condition the PEM membrane. For the NEXIS bottle, this process was further enhanced using laboratory-specific tools, including a 5 mL laboratory syringe fitted with an 18-gauge needle, to inject warm distilled water directly into the anode pinhole at the base of the bottle. This approach was designed to ensure adequate hydration and conditioning of both the cathode and anode sides of the PEM membrane, as shipping and storage conditions may not reliably maintain full membrane hydration on the anode side.

Following this enhanced conditioning protocol, higher dissolved hydrogen concentrations were observed, suggesting that this method may more accurately reflect the bottle's maximum performance potential when the PEM membrane is operating at optimal or peak efficiency. However, consumers should be aware that these results may not be directly replicable under typical use conditions. The conditioning process applied in this evaluation involved specific laboratory tools, controlled distilled water quality, defined water temperature ranges, and a predetermined number of activation cycles, all of which can influence hydrogen output. Additional factors such as gasket integrity, fill volume, lid design, electrolysis cell assembly and pressure rating, and measurement methodology may further contribute to variation in real-world results.

Based on H₂HUBB's evaluation, consumers may reasonably expect dissolved hydrogen concentrations in the range of approximately 6–7 mg/L (ppm) from this bottle on the 10 minute cycle, depending on variables such as water temperature, fill volume, membrane conditioning state, and general use conditions. While individual results may vary, this device has repeatedly demonstrated the ability to achieve dissolved hydrogen concentrations exceeding 6.0 mg/L under controlled testing conditions, supporting its classification among the highest-performing hydrogen water bottles evaluated by H₂HUBB to date.

Overall, the Ocemida NEXIS Professional Hydrogen Water Bottle is a well-engineered system constructed from safe, food-grade materials and capable of producing consistently high, therapeutically relevant concentrations of dissolved molecular hydrogen within its 270 mL capacity. The manufacturer's safety claims were supported by H₂HUBB's evaluation, and the device's performance meets—and in several respects exceeds—H₂HUBB's objective internal performance standards. No safety concerns were identified during testing, and the system incorporates appropriate safeguards to prevent the formation of undesirable byproducts such as chlorine or ozone in the drinking water. Based on our findings, the Ocemida NEXIS represents a safe, high-performing, and reliable option for in-home hydrogen water therapy, offering consumers a combination of strong usability and clinically meaningful hydrogen dosing.

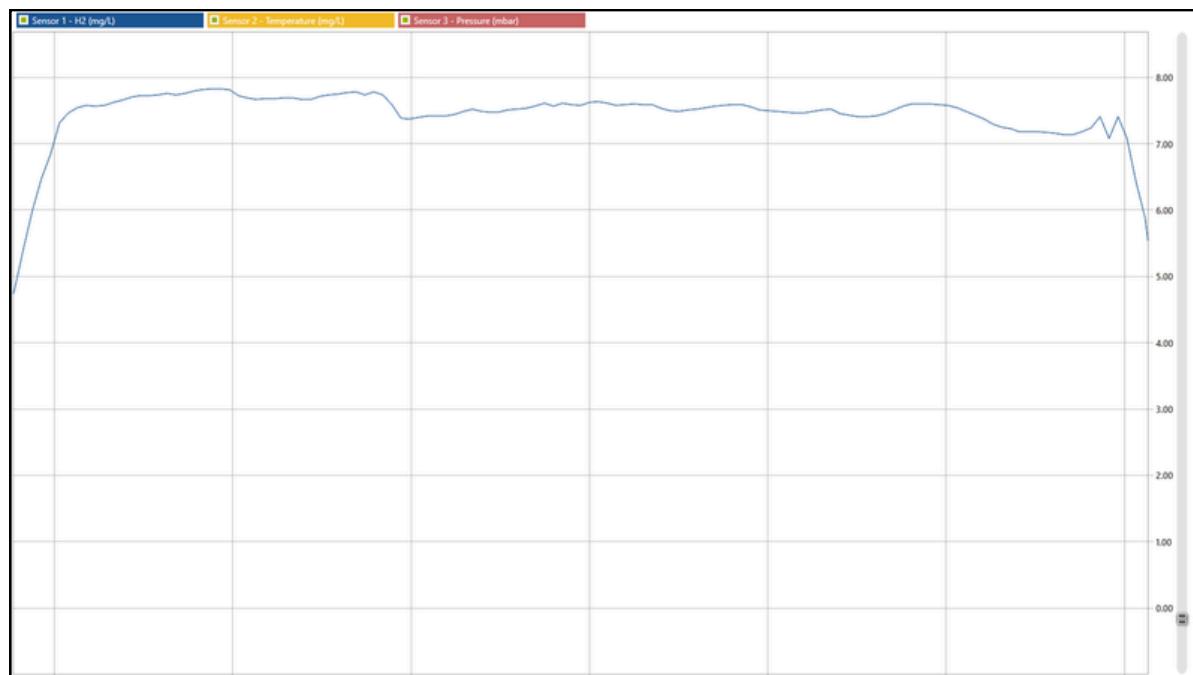


Figure 1. 10-Minute Dissolved H₂ Time-Trace – Ocemida NEXIS Bottle (Unisense H₂ Microsensor)

This plot displays the real-time amperometric output from the Unisense H₂ Microsensor paired with the UniAmp amplifier during a 10-minute hydrogen generation cycle of the Ocemida NEXIS - Professional Hydrogen Water Bottle. The sensor signal, measured in picoamperes and converted to mg/L hydrogen, captures the dynamic dissolved H₂ concentration in the water in real time with a temporal resolution as fine as 0.02 seconds per data point. Data were recorded over the course of the test period, typically 4–5 minutes following bottle opening.

The trace illustrates both the steady-state hydrogen concentration and the natural signal fluctuations that occur during the precipitation phase, as dissolved hydrogen gas begins to equilibrate and outgas from the solution. Due to the high hydrogen concentration and resulting microbubble formation, occasional signal spikes were observed (a known artifact in high-H₂ solutions). To minimize this effect, H₂HUBB employed a controlled re-entry technique—removing and reimmersing the microsensor to dislodge surface bubbles—and then averaged the top 15 stable readings to determine the final dissolved hydrogen value.

This high-resolution time series demonstrates the NEXIS bottle's ability to sustain elevated hydrogen concentrations during and immediately after generation.



H₂ Hubb LLC disclaimer: All tests conducted and test results produced by H₂ Hubb LLC have been done according to industry-accepted practices and standards. Nevertheless, these results may not necessarily reflect test results performed by manufacturers, suppliers or third-party labs. Our test results are independent of all other parties, and testing by other parties may produce different results. We understand that many variables are involved in testing, some of which are extremely difficult to control. These reports are not meant or intended for any other purpose but to uphold H₂ Hubb LLC's business practices and to validate the reasons for our recommendations.



Approved By: Tywon Hubbard

TYWON HUBBARD

CEO, H₂HUBB LLC



Overland Park, KS



www.H₂HUBB.com



info@H₂HUBB.com